

# Your Trauma & Extremities options

## Clavicle

- VariAx 2 Clavicle Plating System

## Elbow

- VariAx 2 Elbow Plating System
- AxSOS 3 Plating System
- Hoffmann 3 External Fixation System
- Hoffmann II Compact MRI External Fixation
- Dynamic Joint Distractor II
- rHead Plating System
- Asnis III Cannulated Screws

## Pelvis

- PRO: Pelvis Reduction & Osteosynthesis Plating System
- Matta Pelvic Plating System
- Hoffmann 3 External Fixation System
- AxSOS 3 Plating System
- Asnis III Cannulated Screws
- Triax Monotube System

## Femur


- ADAPT for Gamma3
- Gamma3 Nailing System
- T2 Nailing Platform System
- T2 Alpha nailing system
- AxSOS 3 Plating System
- Hoffmann 3 External Fixation System
- Hoffmann LRF Circular External Fixation System
- Omega3 Compression Hip Screw System
- Triax Monotube System
- Asnis III Cannulated Screws

## Foot & Ankle

- STAR Total Ankle
- VariAx 2 Foot Plating System
- AxSOS 3 Ankle Fusion System
- Anchorage 2 CP Plating System
- T2 ICF Intramedullary Nail
- T2 Ankle Arthrodesis Nail
- Hoffmann 3 External Fixation System
- Hoffmann LRF Circular External Fixation System
- Hoffmann II Micro and Compact MRI External Fixation System
- Hoffmann LRF Hexapod Deformity Correction
- Triax Monotube System
- Minirail
- Asnis III and Asnis Micro Cannulated Screws
- Asnis JFX System
- Fixos Cannulated Screws
- AutoFIX Cannulated Screws
- TwinFIX
- EasyClip staple system
- EasyStep stepped staple system
- Smart Toe II PIP & DIP implants
- ToeTac hammertoe fixation system
- xFuse System
- SonicAnchor bioresorbable system
- SonicPin bioresorbable system
- EPF Endoscopic Plantar Fasciotomy
- EGR Endoscopic Gastrocnemius Recession
- Asnis Micro Cannulated Screws
- MiNi Cannulated Screws
- Fixos 2 Cannulated Screws

## Utility Plating System

- AxSOS & SPS Basic Fragment Systems (Large Fragment Systems)
- AxSOS & SPS Small Fragment Systems
- VariAx 2 Mini Fragment System

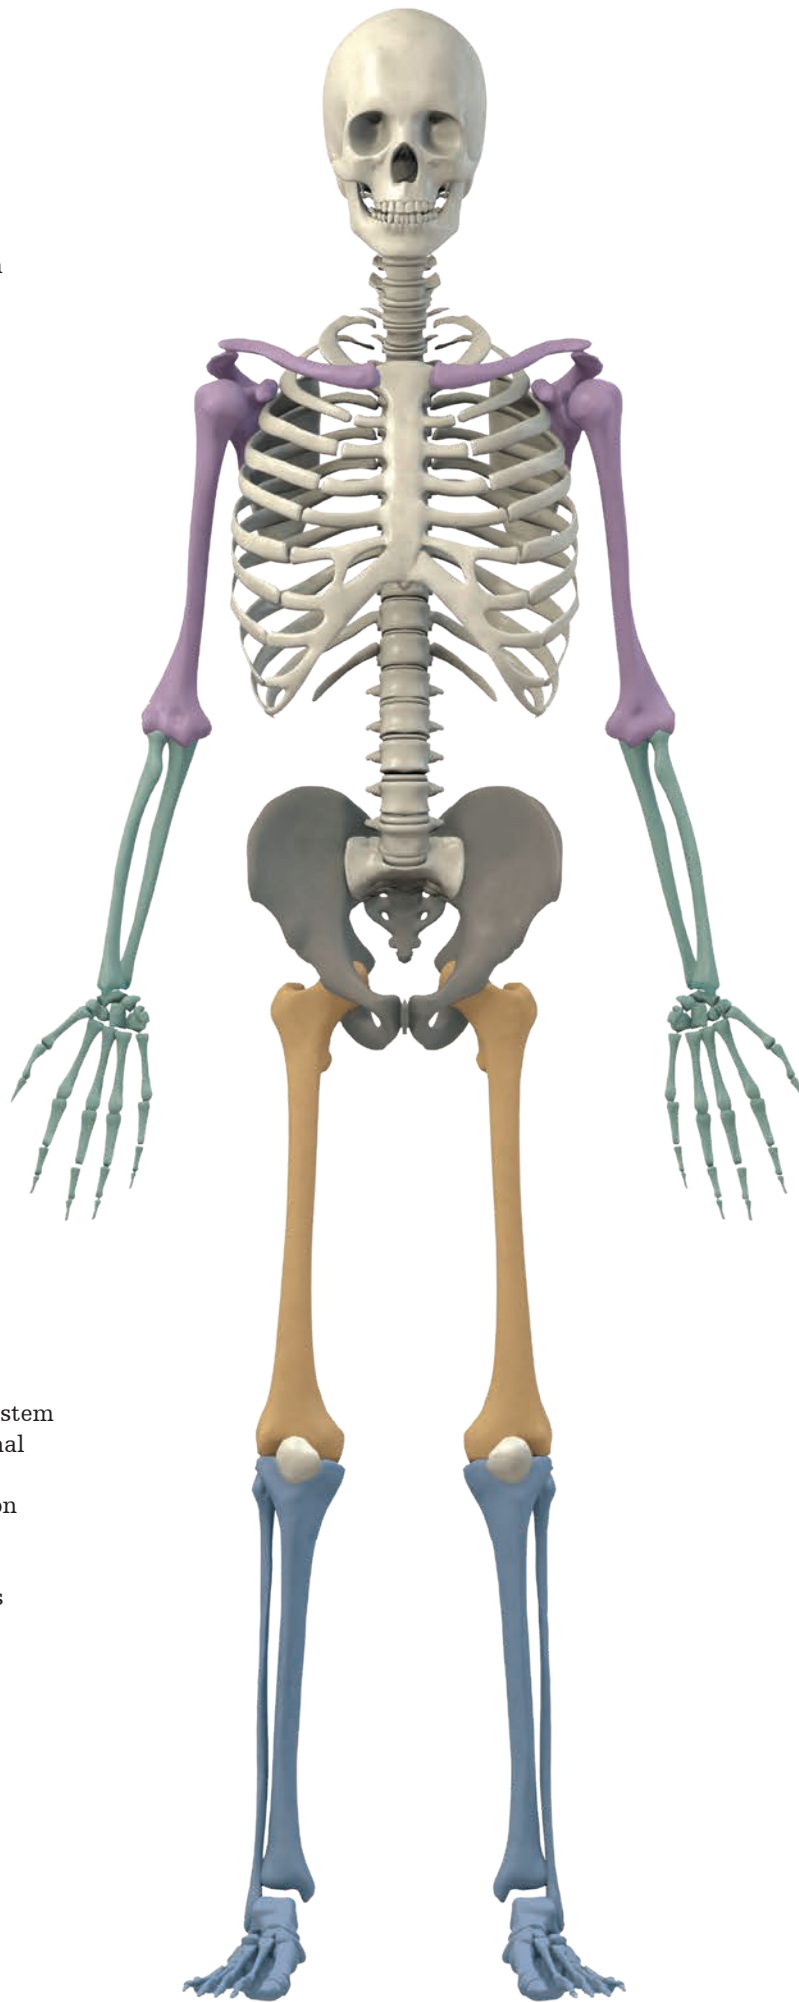

## Humerus

- AxSOS 3 Plating System
- ReUnion Fracture, Total, and Reverse Shoulder System
- T2 Nailing Platform
- Hoffmann 3 External Fixation System
- Hoffmann II Compact MRI External Fixation
- Asnis III Cannulated Screws
- Triax Monotube System

## Forearm

- VariAx 2 Compression Plating System
- AxSOS 3 Plating System
- Hoffmann 3 External Fixation System
- Hoffmann II Compact MRI External Fixation
- Triax Monotube System

## Wrist

- VariAx 2 Distal Radius Plating System
- Hoffmann 3 External Fixation System
- Hoffmann II Compact MRI External Fixation
- Triax Monotube System
- ReMotion Total Wrist System
- Asnis III and Asnis Micro Cannulated Screws
- EasyClip Staple System

## Hand

- VariAx Hand Plating System
- Hoffmann II Micro External Fixation System
- SR PIP and MCP Systems
- Silicone PIP/MCP/MCPX Systems
- Asnis III and Asnis Micro Cannulated Screws
- AutoFIX Cannulated Screws
- Twinfix Cannulated Screws
- ECTR Endoscopic Carpal Tunnel Release
- xFuse System

## Tibia

- AxSOS 3 Plating System
- VariAx 2 Distal Fibula Plating System
- T2 Nailing Platform
- T2 Alpha nailing system
- Hoffmann 3 External Fixation System
- Hoffmann LRF Circular External Fixation System
- Hoffmann LRF Hexapod Deformity Correction
- Asnis III Cannulated Screws
- Triax Monotube System

## Biologics

- Vitoss
- HydroSet XT
- Stryker DBM
- BIO<sup>4</sup>
- AlloWrap DS
- ProLayer
- ProLayer Xenograft
- NeuroMatrix
- Neuroflex
- NeuroMend
- ProChondrix CR
- Traditional Allografts
- Imbibe

# Comprehensive Product Portfolio

## Gamma

Intramedullary Nailing



## T2 & T2 Alpha

Intramedullary Nailing



## Biologics



## VariAx

Small Fragment Plates




## AxSOS

Long Bone Plating



## PRO

Pelvis & Acetabulum Plating

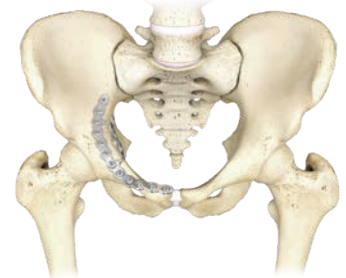


## Anchorage

Plating




## Hoffmann

External Fixation

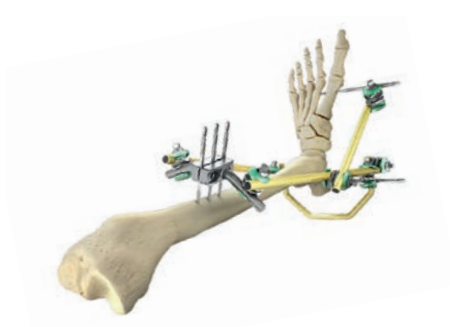

## ReUnion

Shoulder Arthroplasty

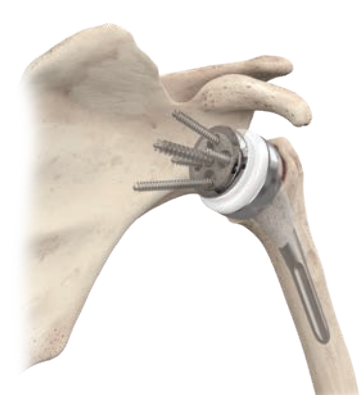

## STAR

Total Ankle



## Asnis

Screw System



## MiNi

Screw System



A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery. The information presented is intended to demonstrate the breadth of Stryker product offerings. A surgeon must always refer to the package insert, product label and/or instructions for use before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area.

Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: Anchorage, Asnis III, AxSOS, AxSOS 3, AutoFIX, BIO4, Dall-Miles, Fixos, Gamma3, Hoffmann, Hydroset, Instratek, Memometal, Monotube, Omega3, rHead, PRO, Re-Motion, ReUnion, STAR, Stryker, T2, Triax, Twinfix, VariAx, Vitoss.

All other trademarks are trademarks of their respective owners or holders.

Allowrap is a registered trademark of Allosource.

Neuroflex, Neuromend, Neuromatrix are trademarks of Collagen Matrix, Inc.

The SR MCP and PIP Arthroplasty System is sold as a HUMANITARIAN USE DEVICE in the US. The effectiveness of this device for this use has not been demonstrated.

Content ID: CP-PO-1, 06-2020

Copyright © 2020 Stryker